


SUPPLEMENTARY FIGURE

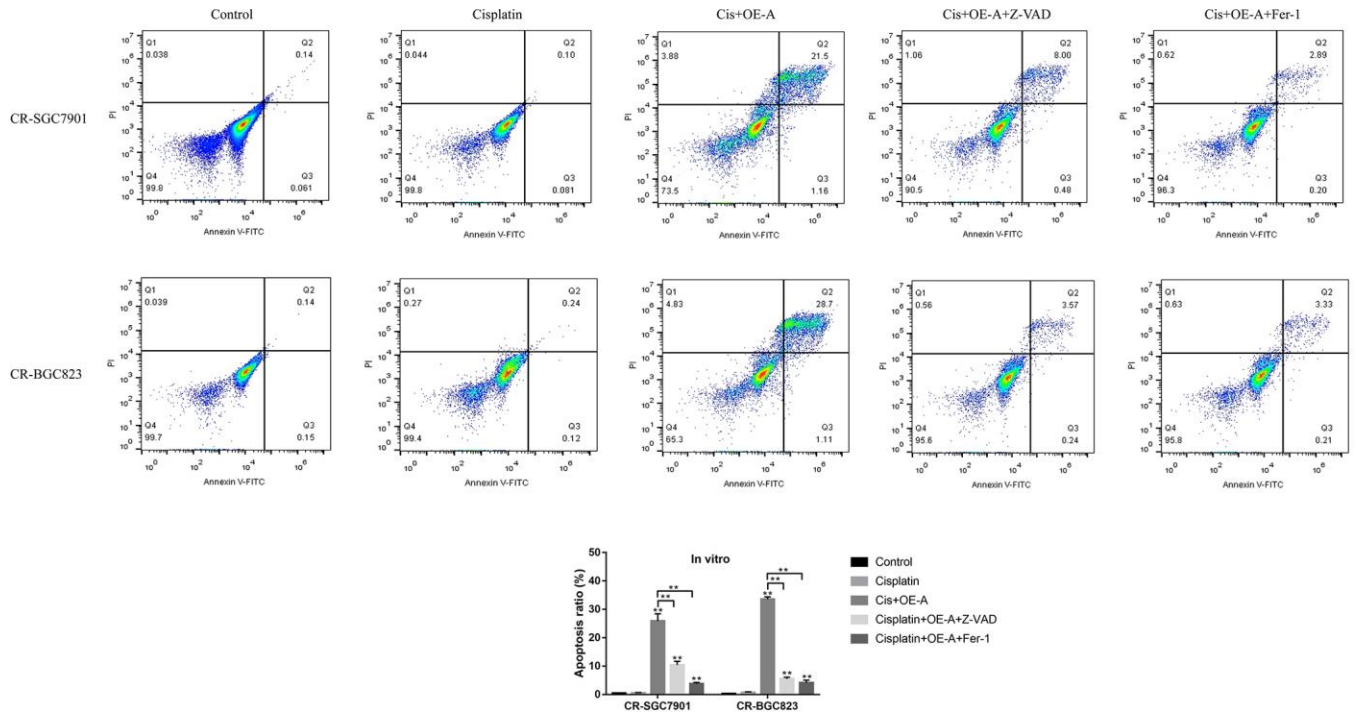

Supplementary Figure 1. FCM assay was performed to detect cell apoptosis ratio. The cells were stained with PI and Annexin V-FITC, and cell apoptosis was measured by FCM. ****P < 0.01.**